

# Design of Impedance Matching Networks for NMR and NQR Studies in the HF Band

Allen Majewski  
Morgan Walker

Department Of Physics, University of Florida  
2001 Museum Rd. Gainesville, FL 32611

September 4, 2016

## Abstract

For more than two decades [3], room temperature Nuclear Quadrupole Resonance (NQR) has been investigated for land mine and general explosives detection due to its ability to unambiguously identify molecular structures, but poor S/N and other practical considerations have limited its use. Achieving impedance matching for a magnetic resonance probe that is sufficiently broad band and well within the dynamic range of real capacitors can be problematic for low frequency magnetic resonance studies of any kind - NQR or low field NMR. Tuning and matching is often done by hand since automation in a two parameter space is non-trivial. Furthermore, designing a probe for the HF band traditionally involves using a coil with a large inductance, which will often ring significantly following a pulse [2], necessitating complex circuitry [1] to dampen the coil's ringing. We explore the use of very low inductance coils for magnetic resonance in the HF band. We present exact solutions for the completely general case of matching an inductive load  $j\omega L + r$  to some characteristic impedance  $Z_0$ , expressing the capacitance values  $C_1, C_2$  individually as functions of  $L, r, \omega$ , and  $Z_0$  and provide software [5] for analysis. Furthermore, we show there is a condition which forces  $C_1 = C_2$  for all  $\omega, L, r$ , effectively reducing the number of free parameters from two to one,

resulting in impedance matching as a one dimensional optimization problem.

## 1 Introduction

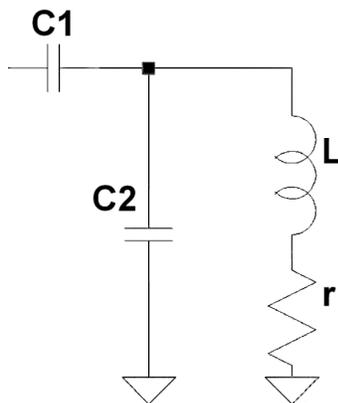


Figure 1: A typical matching topology in NMR which can be solved exactly.

Without cryogenics or the need for large magnetic fields, room temperature table-top NMR and on home-made RF spectrometers offers high modularity of the systems and low cost. However, the design of sufficiently sensitive probes for room temperature NMR or NQR studies in the HF band requires careful selection of components for coil tuning and impedance matching between the transmitter and the sample. For a real inductor having a finite  $Q$ , the reflection coefficient and hence the overall S/N depends on the precise adjustment of two capacitances in a non-linear fashion. For experiments not performed at fixed frequency, such as searching for an unknown NQR, the feasibility of tuning and matching can be prohibitively difficult within the dynamic range of actual capacitors, requiring frequent tear downs during which irreversible changes are introduced to the design. Most large air-variable capacitors have a dynamic range, when mounted, of about 90 percent of their max value, with the lower bound set by the parasitic capacitance between the rotor and the plates as well as the enclosure. Air gaps are available with max values from a fraction of a pF (10 turn trimmer type) to a maximum of 1nF. The ability of your air gap capacitors constraints the frequency range of operation of a given probe configuration.

We will examine the impedance of an L network to characterize the parameter space of the variables  $C_1$ ,  $C_2$ ,  $\omega$ ,  $L$ ,  $r$ . The usefulness of such a calculation is to be able to predict  $C_1$  and  $C_2$  that result in no reflection for a target frequency and a physical coil whose impedance is presumed to be  $j\omega L + r$ . We express  $C_1$  and  $C_2$  in terms of the  $L, r$  and  $\omega$ , since the NQR experimenter is not free to choose  $\omega$ , and generally  $L$  and  $r$  are not independent. We will compare the results with an approximate solution from literature.

## 2 Preliminaries: the matching condition

We define the matching condition for maximum power transfer so that the impedance looking into the probe tank  $Z_0 = 50 \Omega$ , matching the characteristic impedance  $Z_0$  of the coaxial cables commonly used. To do so we must enforce

$$\begin{aligned} \operatorname{Re}[Z] &= Z_0 \\ \operatorname{Im}[Z] &= 0 \Omega \\ Z_0 &= 50 \Omega \end{aligned} \tag{1}$$

Where under typical laboratory conditions,  $Z_0 = 50 \Omega$ , but is not constrained this in analysis. The total impedance looking into the tank ?? is

$$Z = \frac{1}{\frac{1}{j\omega L + r} + j\omega C_2} - \frac{j}{\omega C_1} \tag{2}$$

Because the second term in the expression for  $Z$  has no real part, so we can treat the first term only to find  $\operatorname{Re}[Z]$  and work backwards to express  $\operatorname{Im}[Z]$

$$\frac{1}{jC_2\omega + \frac{1}{r+jL\omega}} = j\omega \frac{L(1 - C_2L\omega^2) - C_2r^2}{(1 - \omega^2LC_2)^2 + (\omega C_2r)^2} + \frac{r}{(1 - \omega^2LC_2)^2 + (\omega C_2r)^2}$$

$$\text{Re}[Z] = \frac{r}{(1 - \omega^2LC_2)^2 + (\omega C_2r)^2} \quad (3)$$

$$\text{Im}[Z] = \omega \frac{L(1 - C_2L\omega^2) - C_2r^2}{(1 - \omega^2LC_2)^2 + (\omega C_2r)^2} - \frac{1}{\omega C_1}$$

and so the impedance can be written in the more illuminating form

$$Z = \frac{r}{(1 - \omega^2LC_2)^2 + (\omega C_2r)^2} + j\omega \frac{L(1 - C_2L\omega^2) - C_2r^2}{(1 - \omega^2LC_2)^2 + (\omega C_2r)^2} - \frac{j}{\omega C_1} \quad (4)$$

### 3 Approximate solution

An approximate solution for  $C_1, C_2$  in terms can be obtained [4] by asserting that  $(\omega C_2r)^2$  and  $C_2r^2$  are small, the author neglects these terms reducing the full expansion of the total impedance  $Z$  to

$$Z \approx \frac{r}{(1 - \omega^2LC_2)^2} + j\omega \frac{L}{(1 - \omega^2LC_2)} + \frac{1}{j\omega C_1} \quad (5)$$

Setting  $Z = Z_0$  and recognizing that  $Z_0$  is real, we can express  $C_2$  at the matching condition immediately

$$C_2 \approx \frac{1 - \sqrt{r/Z_0}}{\omega^2 L} \quad (6)$$

and similarly,  $C_1$  is obtained with  $\text{Im}[Z] = 0$

$$C_1 \approx \frac{\sqrt{r/Z_0}}{\omega^2 L} \quad (7)$$

it follows that at the matching condition,  $r$  can be expressed in terms of  $Z_0, C_1, C_2$  alone

$$r \approx \frac{Z_0}{\left(1 + \frac{C_2}{C_1}\right)^2} \quad (8)$$

and is worth noting that if  $r$  is set to exactly  $Z_0/4$ , then  $C_1 = C_2$  when the circuit is tuned and matched, regardless of  $L$ ,  $\omega$ , or  $Z_0$ .

## 4 An exact solution

Looking back to equation 3,  $\text{Re}[Z]$  is quadratic in  $C_2$  and has no dependence on  $C_1$ , so we can solve for  $C_2$  outright. With  $\text{Re}[Z] = Z_0$  we find

$$\frac{r}{Z_0} = C_2^2 (L^2\omega^4 + r^2\omega^2) - 2C_2L\omega^2 + 1 \quad (9)$$

We can now express  $C_2$  in terms of  $L$ ,  $\omega$ , and  $r$  and  $Z_0$  only by solving the quadratic

$$C_2^\mp = \frac{L\omega^2 Z_0 \mp \sqrt{L^2 r \omega^4 Z_0 - r^2 \omega^2 Z_0^2 + r^3 \omega^2 Z_0}}{L^2 \omega^4 Z_0 + r^2 \omega^2 Z_0} \quad (10)$$

Returning to equation 3, we examine  $\text{Im}[Z]$

$$\text{Im}[Z] = \omega \frac{L(1 - C_2 L \omega^2) - C_2 r^2}{(1 - \omega^2 L C_2)^2 + (\omega C_2 r)^2} - \frac{1}{\omega C_1} \quad (11)$$

which we set to zero and immediately solve for  $C_1$  in terms of  $C_2$

$$C_1 = \frac{1}{\omega^2} \frac{(1 - \omega^2 L C_2)^2 + (\omega C_2 r)^2}{C_2 r^2 + C_2 L^2 \omega^2 - L} \quad (12)$$

Inserting each of the two roots of equation 9 into 12 gives

$$C_1^\mp = \pm \frac{r}{\sqrt{r \omega^2 Z_0 (L^2 \omega^2 + r^2 - r Z_0)}} \quad (13)$$

The negative value of  $C_1$  is nonsense, confirming that  $C_2^-$  is the valid solution from the quadratic in  $C_2$  - thus,  $C_2^+$  should be thrown out leaving us with

exact expressions for  $C_1, C_2$  in terms of  $Z_0, L, \omega, r$ :

$$\begin{aligned}
C_2 &= \frac{L\omega^2 Z_0 - \sqrt{L^2 r \omega^4 Z_0 - r^2 \omega^2 Z_0^2 + r^3 \omega^2 Z_0}}{L^2 \omega^4 Z_0 + r^2 \omega^2 Z_0} \\
C_1 &= \frac{1}{\omega^2} \frac{(1 - \omega^2 L C_2)^2 + (\omega C_2 r)^2}{C_2 r^2 + C_2 L^2 \omega^2 - L} \\
&= \frac{r}{\sqrt{r \omega^2 Z_0 (L^2 \omega^2 + r^2 - r Z_0)}}
\end{aligned} \tag{14}$$

Though calculation was motivated by applications in the HF-VHF band, the results assume nothing about parameters' magnitudes.  $Z_0$  is not limited to  $50\Omega$ , and the capacitances are not assumed to be small. No approximations were made limiting the frequency of operation.

## 5 Comparison of approximate and exact expressions

The approximate solution obtained showed at the matching condition

$$\begin{aligned}
C_1 &\approx \frac{\sqrt{r/Z_0}}{\omega^2 L} \\
C_2 &\approx \frac{1 - \sqrt{r/Z_0}}{\omega^2 L}
\end{aligned} \tag{15}$$

By reannanging the to exact expression for  $C_2$  we can compare the results

$$\begin{aligned}
C_2 &= \frac{L\omega^2 Z_0 - \sqrt{L^2 r \omega^4 Z_0 - r^2 \omega^2 Z_0^2 + r^3 \omega^2 Z_0}}{L^2 \omega^4 Z_0 + r^2 \omega^2 Z_0} \\
&= \frac{1 - \sqrt{r/Z_0 - r^2/(\omega^2 L^2) + r^3/(\omega^2 Z_0 L^2)}}{\omega^2 L + r^2/L}
\end{aligned} \tag{16}$$

and similliarly for  $C_1$

$$\begin{aligned}
C_1 &= \frac{r}{\sqrt{r\omega^2 Z_0 (L^2 \omega^2 + r^2 - rZ_0)}} \\
&= \frac{\sqrt{r/Z_0}}{\omega^2 L} \frac{1}{\sqrt{1 - r(Z_0 - r)/(L^2 \omega^2)}}
\end{aligned} \tag{17}$$

|                                       |   |
|---------------------------------------|---|
| Approximate $C_1$                     | Exact $C_1$   |
| $\frac{\sqrt{r/Z_0}}{\omega^2 L}$     | $\frac{\sqrt{r/Z_0}}{\omega^2 L} \frac{1}{\sqrt{1 - r(Z_0 - r)/(L^2 \omega^2)}}$            |
| Approximate $C_2$                     | Exact $C_2$   |
| $\frac{1 - \sqrt{r/Z_0}}{\omega^2 L}$ | $\frac{1 - \sqrt{r/Z_0 - r^2/(\omega^2 L^2) + r^3/(\omega^2 Z_0 L^2)}}{\omega^2 L + r^2/L}$ |

We see that the exact value of  $C_1$  at the matching condition can be seen as the approximate result from Jiang, multiplied by a correction factor  $\frac{1}{\sqrt{1 - r(Z_0 - r)/(L^2 \omega^2)}}$ .

The situation for  $C_2$  is somewhat more complicated.  $C_2$  will be very close to the approximate result when  $L$  is relatively large,  $Z_0$  dominates  $r$ , or both.

## 6 Results

The approximate expressions for  $C_1$ ,  $C_2$  are in general most accurate when  $Q = L\omega/r$  is high. Conversely, there is a large margin of error for arrangements with a  $Q < 50$ . The most interesting cases are when the approximate solutions fail when  $Q$  is at least 50, as a  $Q$  of 50 is a typical value for NMR or NQR experiments. These situations occur on the boundary of mathematically acceptable values of  $L$ . If  $L$  is low, the error in  $C_1$  can exceed ten percent even when  $Q > 50$ . For example,  $f = 1.7$  MHz,  $L = .5 \mu\text{H}$ ,  $r = .1 \Omega$  gives  $Q = 52$  and an error in the value of  $C_1$  of .103 (exceeding ten percent).

| $f$ (MHz) | $L$ ( $\mu\text{H}$ ) | $r$ ( $\Omega$ ) | $Q$   | $C_1$ error | $C_2$ error |
|-----------|-----------------------|------------------|-------|-------------|-------------|
| 1.7       | .500                  | .102             | 52.35 | .103        | .00406      |
| 2.7       | .330                  | .110             | 50.89 | .101        | .00419      |
| 3.3       | .270                  | .111             | 50.44 | .102        | .00418      |
| 4.3       | .200                  | .104             | 51.96 | .103        | .00408      |
| 5.3       | .129                  | .0827            | 51.92 | .135        | .00467      |
| 29.92     | .03                   | .111             | 50.81 | .100        | .00412      |
| 200.3     | .002                  | .0239            | 105.3 | .110        | .00212      |

Selected cases with  $Q > 50$  and error of  $C_1$  value in excess of ten percent. Calculated with capMatch.py [5]

From equation (15), a very interesting relationship can be seen. If  $r = \frac{Z_0}{4}$ , then  $C_1 = C_2$  for all  $\omega, L$ . In practice, a coil is fabricated and the losses are measured - it is difficult to control  $r$  with much accuracy. Nevertheless, if this condition were to be met, the number of free parameters for achieving the matching condition would be reduced from two to one. This would make automated tuning trivial, as compared with the case of having two capacitances to match, in which a sophisticated control system is required for sweeping.

## 7 Summary

We provide exact expressions for the values of capacitance that satisfy the matching condition for a typical L-network used in NMR and NQR probes for HF and VHF frequencies. We showed that the previously known approximate solutions can fail to accurately compute capacitances at the matching condition when  $L$  is sufficiently low, even in cases where  $Q$  exceeds 50.

This work was supported in part by the National High Magnetic Field Laboratory funded by the NSF (DMR-1157490) and the State of Florida.

## References

- [1] M. S. Conradi. Fet q switch for pulsed nmr. *Review of Scientific Instruments*, 48(3):359–361, 1977.
- [2] E. Fukushima and S. Roeder. Spurious ringing in pulse nmr. *Journal of Magnetic Resonance (1969)*, 33(1):199–203, 1979.
- [3] A. N. Garroway, M. L. Buess, J. P. Yesinowski, J. B. Miller, and R. A. Krauss. Explosives detection by nuclear quadrupole resonance (nqr). In *SPIE's 1994 International Symposium on Optics, Imaging, and Instrumentation*, pages 139–149. International Society for Optics and Photonics, 1994.
- [4] Y. J. Jiang. A simple method for measuring the q value of an nmr sample coil. *Journal of Magnetic Resonance*, 142(2):386–388, 2000.
- [5] A. R. Majewski. <https://github.com/altoidnerd/capmatch>. *GitHub Repository*, 2015.